


DISTORTION METER

9/12/58


Given: 50 kc
0.75 mc
1.65 mc
4.0 mc

Req'd: A means of measuring the above freq. total amount of harmonic distortion. To be used on Tek Type 190 or similar sine wave generator.

Method: Use a Bridged "T" null network of the basic design shown in Figure 1. (below)

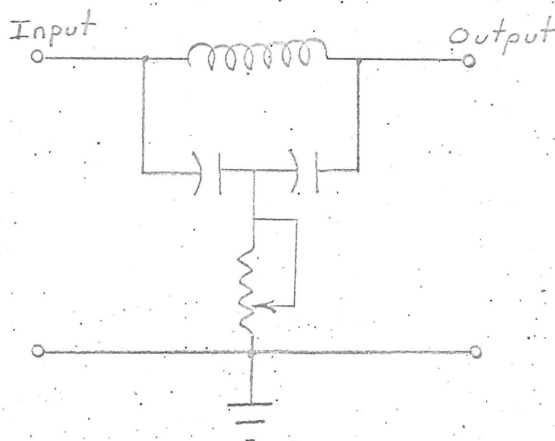

Range Switch

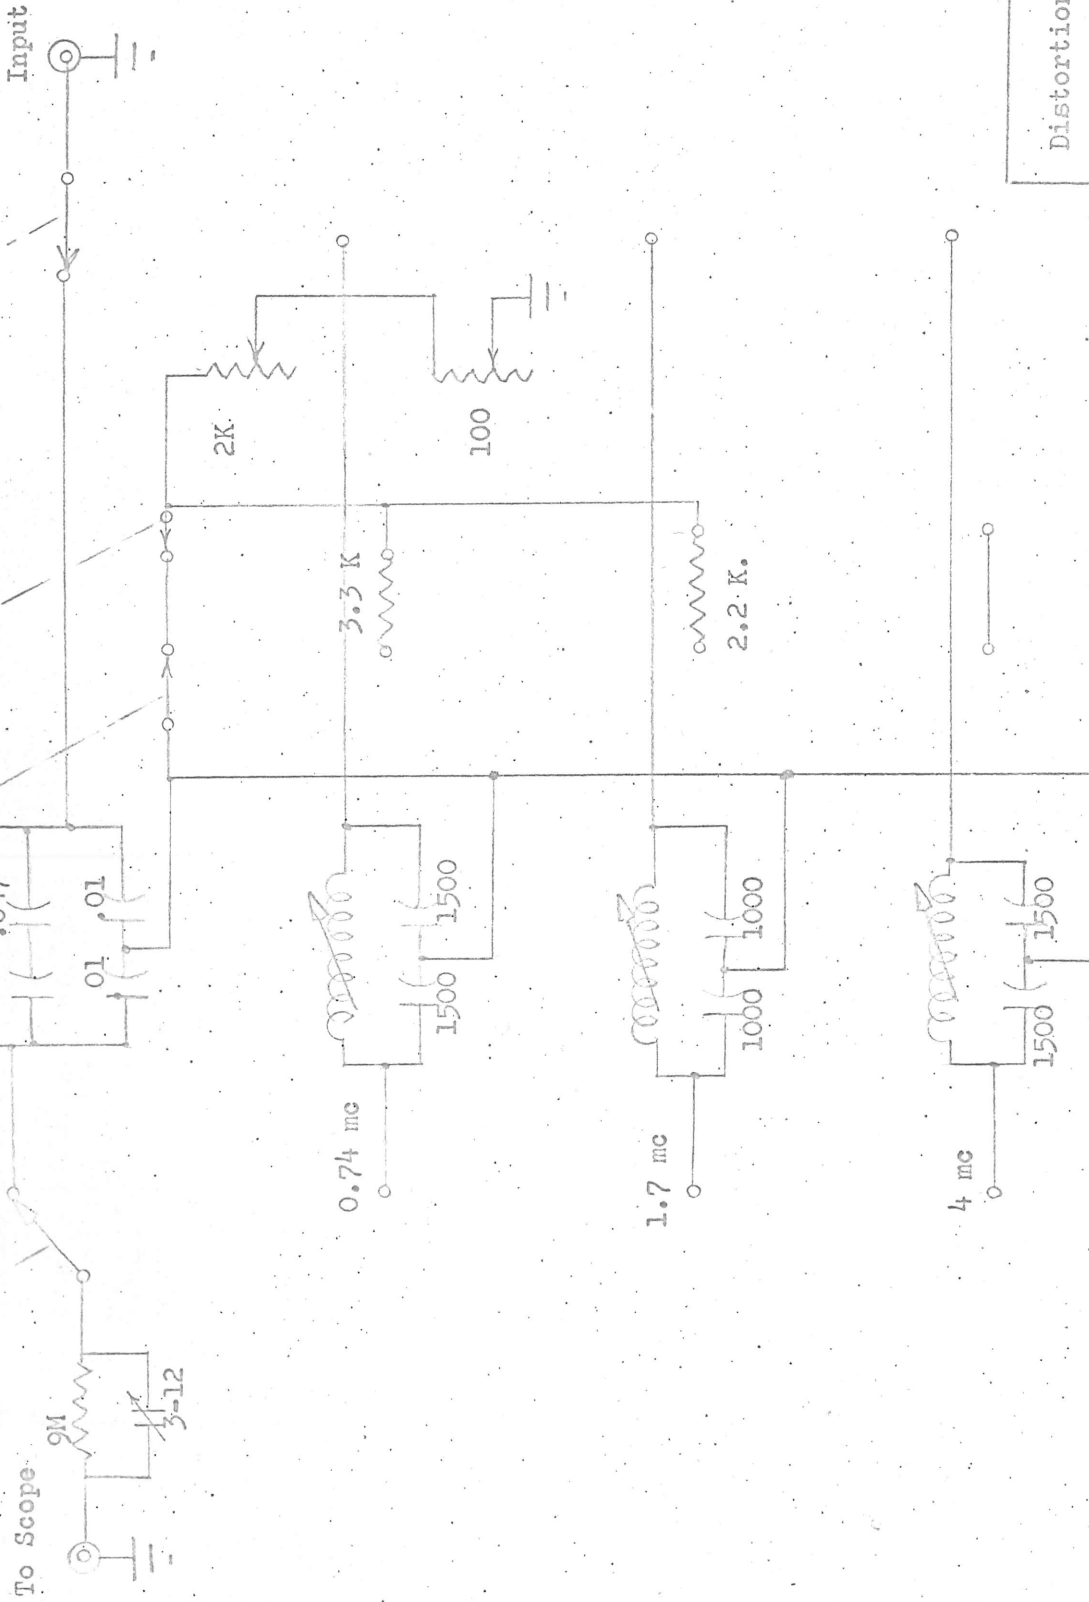

Distortion Meter

Tektronix Inc. Prod. Elec.

9/12/58

J.L. Stoll